

Super Canister Instructions v3.0

Standard Model with magnetic safety coupling.

Introduction

The Supercanister Model is a foreskin restoration tugging device. The device allows tensioning of the penis skin tube to reverse circumcision by skin expansion. The device allows the glans (head) to partially recess inside, and is narrower than other canister designs. Once attached, the device permits urination without removal. Each Supercanister is precision machined by ADI from a solid billet of food-grade Dupont polymer. The device incorporates an integral magnetic safety coupling which will detach in the event of excessive tension, preventing injury to the penis. Under normal levels of tension, the coupling will stay attached. The safety coupling's swiveling design will also prevent the penis from being subjected to torsion or twisting. The Supercanister features a narrowing tapered cone which helps to create a narrow and conforming restored foreskin.




To apply the Supercanister:


1. Obtain a 10" (25cm) long by 2" (50mm) wide strip of surgical tape.




2. Apply Adhesi-Med (TM), either brush-on or spray, to tapered area of device and allow up to 1 minute drying time. Avoid getting Adhesi-Med near the edge of the cone.

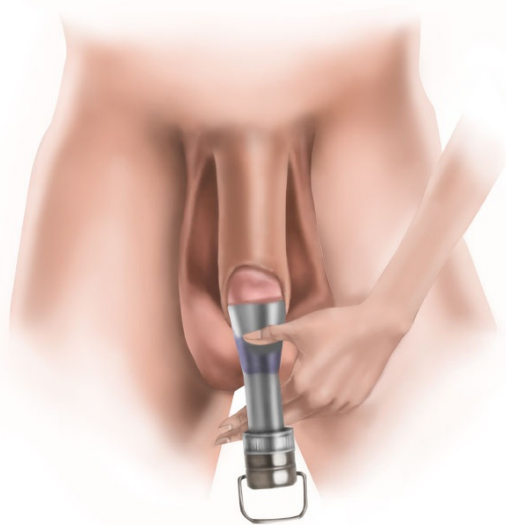


3. Take lower skin and pull it over device, and press against device until adhesive sets.

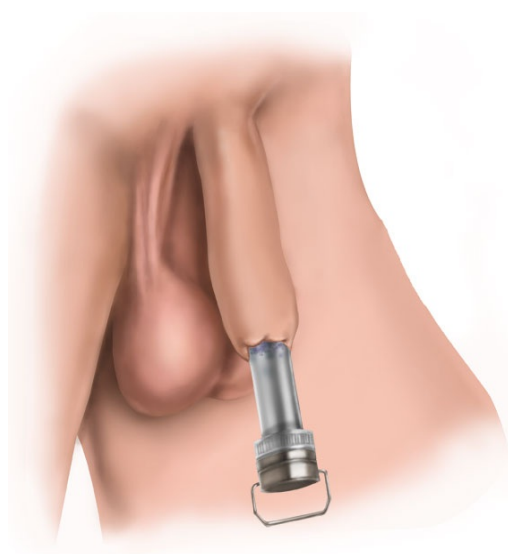

4. Pull top skin over device until adhesive sets. Pull sides up and squeeze for several seconds until skin is firmly bonded to adhesive..

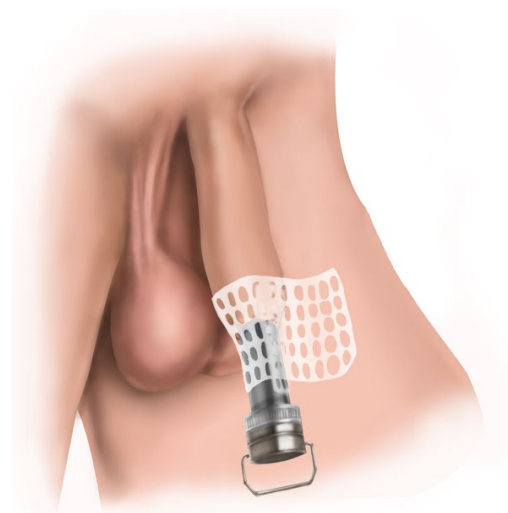

5. Begin taping the foreskin to the device. This first wrap should come in contact with both skin and the barrel. Wrap tape over 3/8" to 1/2" of skin.

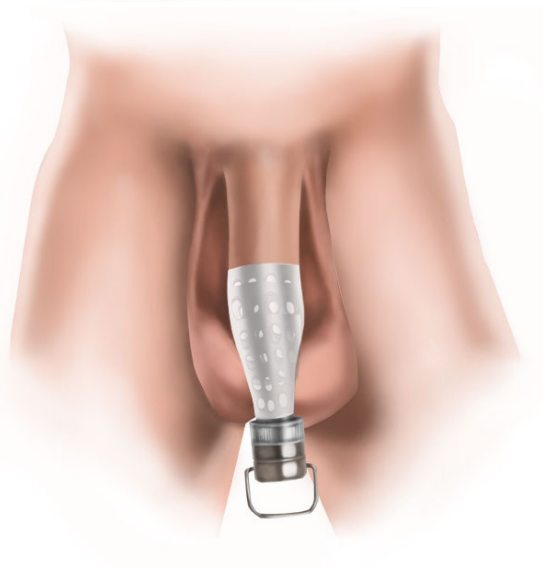

6. Continue to wrap all of the tape around the device. Be sure to cover over any skin folds. Be sure to use 2" (50mm) width tape. With each wrap, advance the tape slightly 1/8" (3mm) cover additional skin farther up the shaft. Before completely wrapping, fold back the end of the tape to facilitate later removal. Wrap carefully with moderate pressure to avoid leaks.

As your new foreskin restores, you may advance the skin higher up the device and depress the glans with the cone when applying the device. This will provide "bi-directional" tension. You may advance the skin all the way up to the collar and secure with 1" tape.

7. Attach Advanced Device's Torpedo Tugging weights to the bail, and tug with light to moderate pressure.. Our Torpedo weights are very effective, available on our website www.shop.foreskin-restoration.info

8. To urinate, simply disconnect strap or move out of way, hold barrel and urinate normally. If stream is erratic, gently pull on device to align urethral opening with drain hole. Shake out remaining urine when done. Insert disposable cotton roll to absorb any remaining urine and prevent soiling of clothing.

8. If you feel minor discomfort, disconnect weight and take a 15 minute break.

9. To remove device, spray Citri-Med (TM) Citrus Adhesive and Tape remover onto tape. This will cause the tape to immediately release. Slowly remove tape without harming skin.

Foreskin Restoration suggestions:

Foreskin restoration can be accomplished with comfort and convenience. While you can experiment to see which is best for you, we suggest the following:

1. Tug for 8-12 hours per day, 3 to 5 days per week. Take at least 2 days per week off to allow the skin to repair and regrow.
2. Tug with moderate weight. You are using too much tension if you get bruises or skin tears. In this event, take several days off from tugging to allow the skin to heal. Re-start tugging after healing with lower tension levels.
3. Use quality tape. The tape we make available from our webstore has been tested to ensure its performance with our devices. Other types or brands of tape may not securely hold the device in place, or allow urine leakage.

Warnings:

1. Do not sleep while wearing any foreskin restoration device.
2. Do not exceed 17 ounces of tugging force.
3. If you feel any pain discontinue use immediately .
4. Consult with a medical professional before attempting foreskin restoration.
5. Wash the Supercanister inside and out with soap and water after each use.
6. Do not wear the Supercanister when operating machinery or other potentially hazardous conditions.
7. This device uses an extremely strong magnet. Do not use if you wear a pacemaker. Do not place the magnet near electronic devices or media.



www.foreskin-restoration.info

For online support join our forum at
www.foreskin-restoration.info/forum

"Helping you reach your goals"